

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

JAN 19 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130526
Name		JOSEPH V. SHOEMAKER	ID# 4188 Date 1-14-09
A	Agency	(SDPI) SAND Point P.D.	Phone # 383-3700
Instrument Location		SAND Point, AK 99661	
Alco S/N		X173004	Target Value .079 High Pressure 600
Alco Test Value Average		0.075 1st Alco	0.076 2nd Alco
Signature		Joseph V. Shoemaker	
		(OVER)	


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 20th day of January, 2010.
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

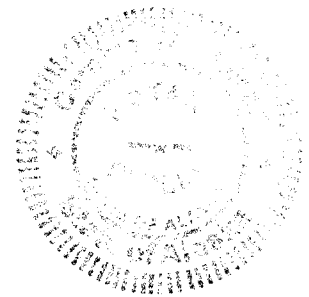

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130526

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130526

JANUARY 14, 2010

OPERATOR'S NAME: *AS 1/22/10*
SHOEMAKER J V
OPERATOR'S NUMBER: 4188
SUBJECT'S LAST NAME:
K
SUBJECT'S FIRST NAME/MI :
K
O.L. #: K
DEPT/AGENCY: SDPI
CASE/REPORT: D
TEST TYPE: V
ALCO TARGET VALUE: .079
ALCO S/N: K173004

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.34 in		
ALCO TARGET	.077	13:10
BLANK TEST	.000	13:11
INTERNAL STANDARD	VERIFIED	13:11
ALCO TV 29.34 in	.075	13:11
BLANK TEST	.000	13:12
SUBJECT SAMPLE	.000	13:13
BLANK TEST	.000	13:14
ALCO TV 29.34 in	.076	13:14
BLANK TEST	.000	13:15

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130526

JANUARY 14, 2010
TIME 13:17

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	41c
BAROMETER:	29.34 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~"